Scan-Thru Workflow for Certain[®] and Ex-Hex[®] BellaTek Abutments



TRIOS® Scanner

Trios scanner must be setup to send order to customer's 3Shape Communicate Inbox prior to scan (this is a one-time setup – contact Customer Service for assistance).

Step 0:

a) Create an order in your Trios Scanner using the following settings:

Restoration: "Crown"

Color: "Gold"Shade: "Vita 1"

Step 1:


b) Double click on the 3Shape icon.





d) Trios order will appear in the "3Shape communicate inbox".

e) Right click on the order, select "Open" to modify order.



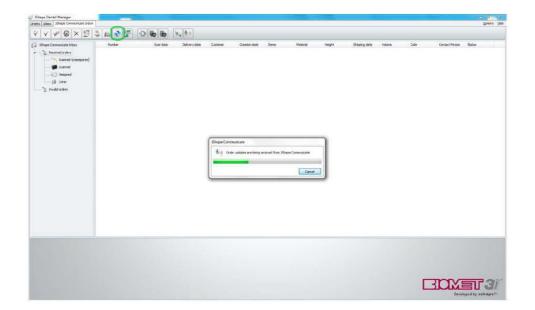

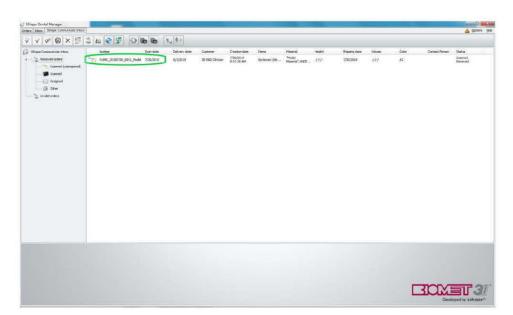


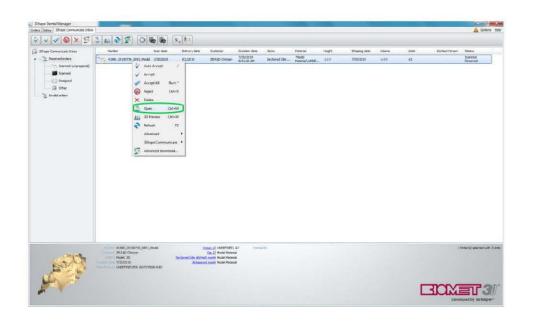

Scan-Thru Workflow for Certain[®] and Ex-Hex[®] BellaTek Abutments




TRIOS® Scanner

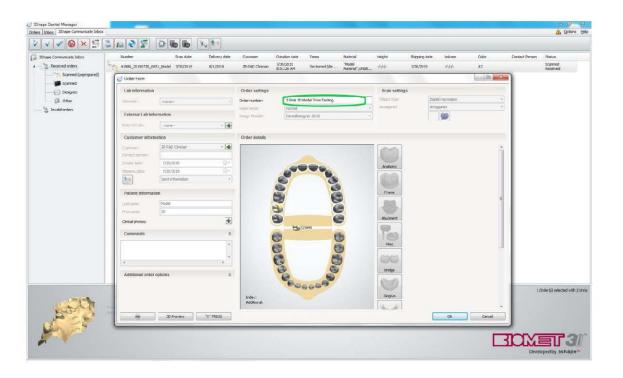

Step 2:

a) Change order number, then click "Ok" to continue.

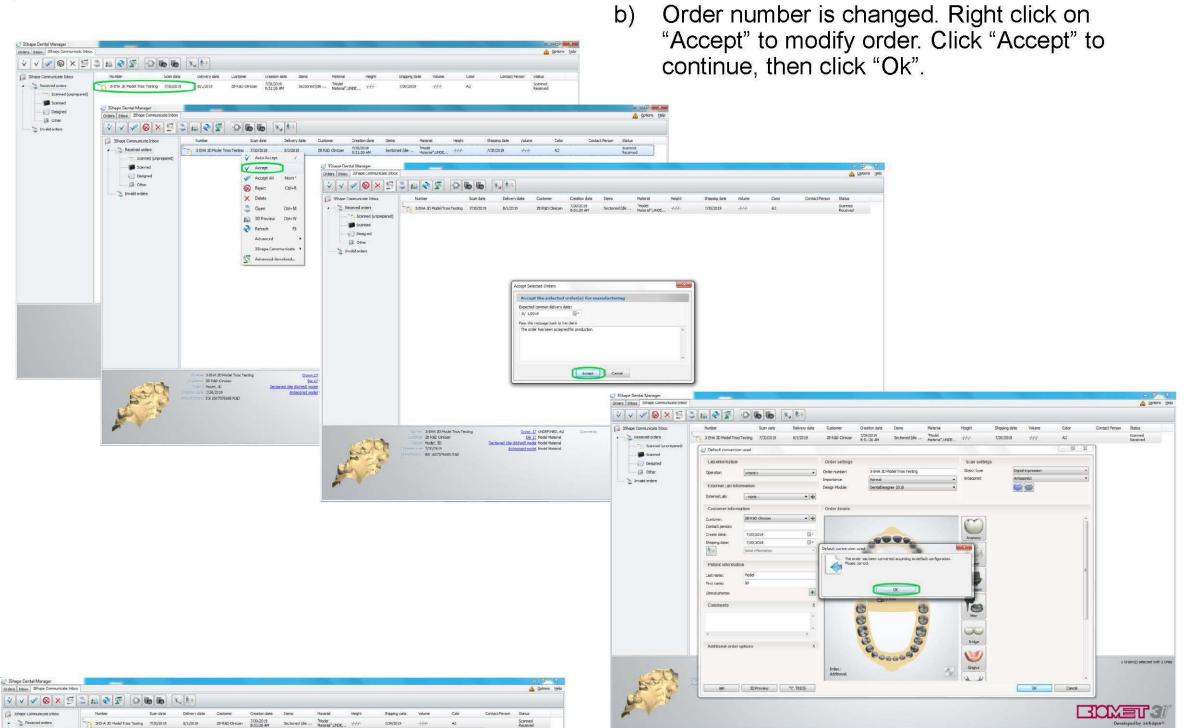

Default conversion used

Some differentiates

Construction

Construction

Control of the construction

Construction

Control of the construction


Control of the


c) Click on tooth to change crown material to "3i EHA 3D Model" material.


Scan-Thru Workflow for Certain[®] and Ex-Hex[®] BellaTek Abutments



TRIOS® Scanner

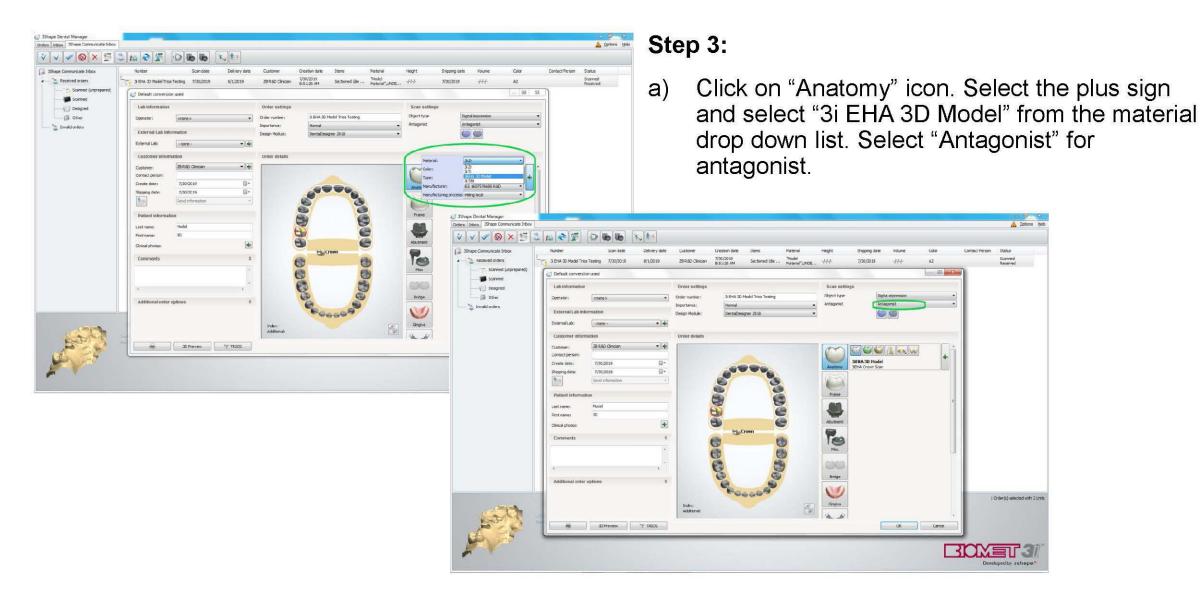

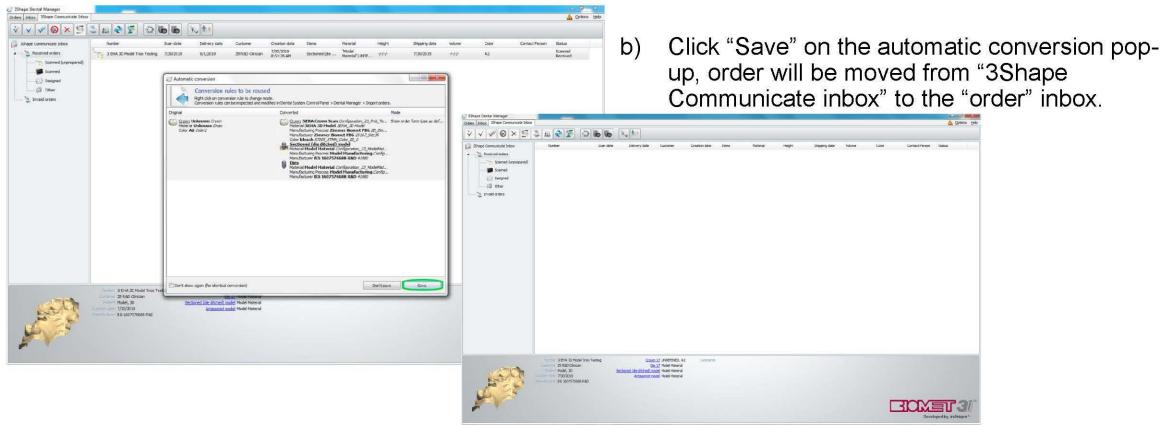

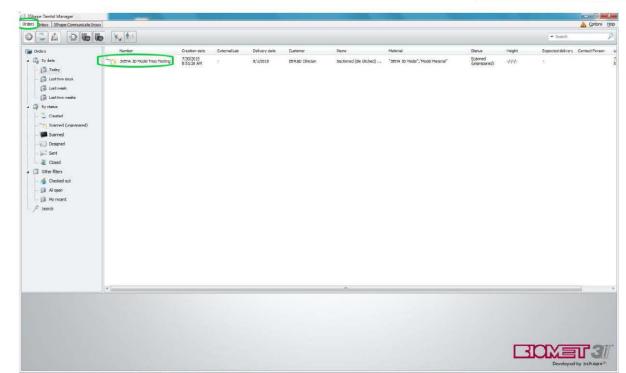

c) Order will appear in "Orders" inbox.


Scan-Thru Workflow for Certain® and Ex-Hex® BellaTek Abutments





TRIOS® Scanner

Step 4:

Press F4 to open the order folder. Drag or paste the completed pdf BellaTek Work Order form file inside the order folder. Close folder to continue.

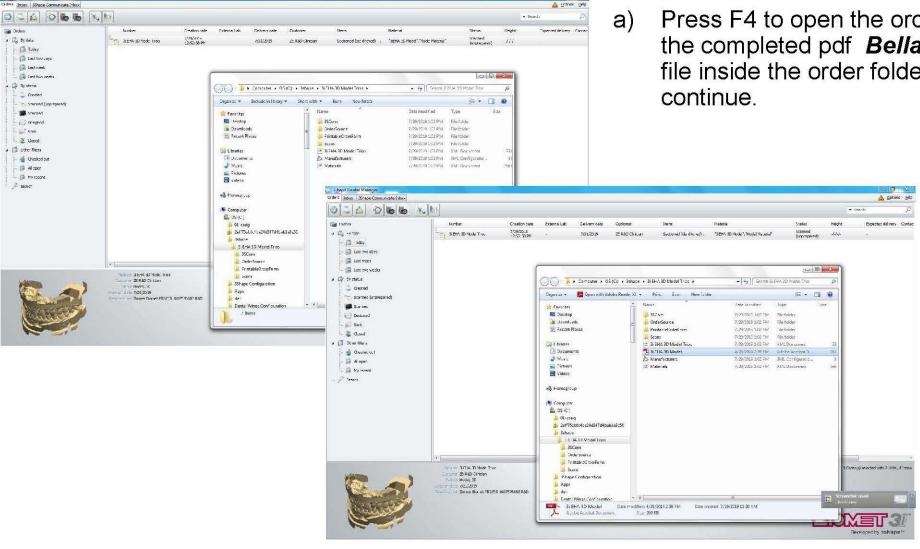

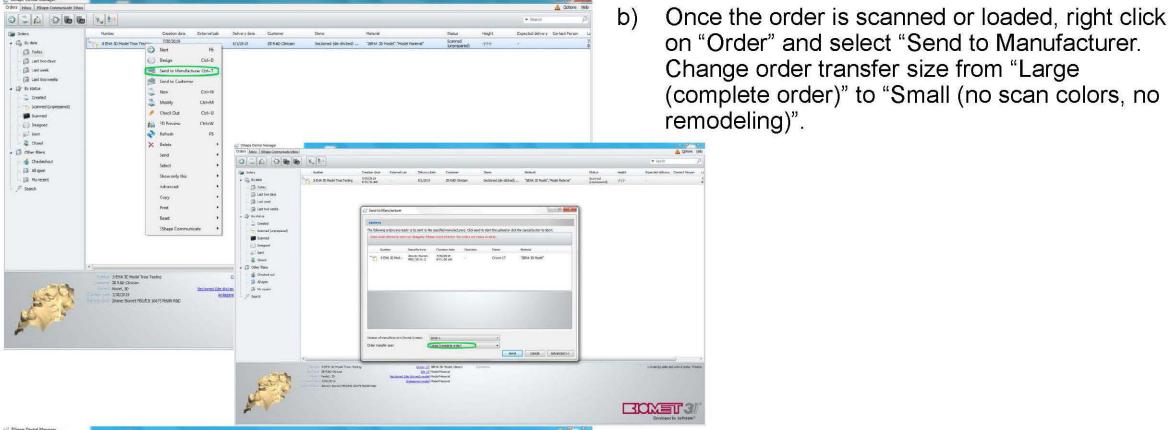

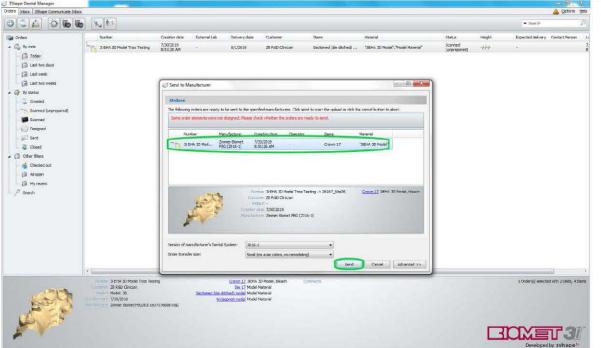

Click on order and then click "Send" to send the order to the manufacturer.

Unless otherwise indicated, as referenced herein, all trademarks are the property of Zimmer Biomet; and all products are manufactured by one or more of the dental subsidiaries of Zimmer Biomet Holdings, Inc. and marketed and distributed by Zimmer Biomet Dental and its authorized marketing partners. For additional product information, please refer to the individual product labeling or instructions for use. Product clearance and availability may be limited to certain countries/regions. This material is intended for clinicians only and does not comprise medical advice or recommendations. Distribution to any other recipient is prohibited. This material may not be copied or reprinted without the express written consent of Zimmer Biomet Dental. Trios is a trademark of 3Shape A/S. ZB0903WF REV C 04/21 ©2021 Zimmear Biomet. All rights reserved.